



A11106 053687

REFERENCE

NIST  
PUBLICATIONS

National Voluntary  
Laboratory Accreditation  
Program



U.S. DEPARTMENT OF COMMERCE  
National Bureau of Standards

# Insulation LAP Handbook

OPERATIONAL AND TECHNICAL REQUIREMENTS  
OF THE  
LABORATORY ACCREDITATION PROGRAM  
FOR  
THERMAL INSULATION MATERIALS

NBSIR 85-3184

U.S. DEPARTMENT OF COMMERCE  
National Bureau of Standards  
Office of Product Standards Policy  
Gaithersburg, Maryland 20899

QC 985  
100  
.U56  
85-3184  
1985



**INSULATION LAP HANDBOOK  
OPERATIONAL AND TECHNICAL REQUIREMENTS  
OF THE  
LABORATORY ACCREDITATION PROGRAM  
FOR  
THERMAL INSULATION MATERIALS**

**NBSIR 85-3184**

**Wiley A. Hall, Jr.  
Robert L. Gladhill  
Jeffrey Horlick  
Harvey W. Berger**

**U.S. DEPARTMENT OF COMMERCE  
National Bureau of Standards  
Office of Product Standards Policy  
Gaithersburg, Maryland 20899**

**June 1985**

**U.S. DEPARTMENT OF COMMERCE, Malcolm Baldrige, *Secretary*  
NATIONAL BUREAU OF STANDARDS, Ernest Ambler, *Director***



Table of Contents

	<u>Page</u>
I. THE INSULATION LAP AT A GLANCE . . . . .	1
II. INTRODUCTION. . . . .	2
III. ADMINISTRATIVE AND OPERATIONAL REQUIREMENTS. . . . .	4
Laboratory Code Number . . . . .	4
Accreditation Period . . . . .	4
Renewal. . . . .	4
Publicizing Accreditation Status . . . . .	4
By NVLAP	
By Laboratories	
Compliance with Existing Laws. . . . .	5
Accreditation Process. . . . .	5
Application and Fees	
Approved Signatory	
Technical Experts	
On-site Assessment	
Monitoring Visits	
Proficiency Testing	
Technical Evaluation	
Administrative Review	
Accreditation Actions. . . . .	10
IV. TECHNICAL REQUIREMENTS . . . . .	11
Scope of LAP . . . . .	11
Quality Assurance System . . . . .	11
Documentation	
Personnel	
Equipment and Facilities	
Maintenance and Calibration	
Proficiency Testing	
Test Methods and Procedures	
Recordkeeping	
Test Reports	
V. PROFICIENCY TESTING. . . . .	16
APPENDICES	
NVLAP Accreditation Criteria (December 1984)	
NVLAP Lab Bulletin No. 3A	
Test Method List	



## I. THE INSULATION LAP AT A GLANCE

This document presents the operational and technical requirements of the Laboratory Accreditation Program (LAP) for thermal insulation materials. All of the steps leading to accreditation are described. Technical requirements are explained indicating how the NVLAP criteria are applied.

The laboratory accreditation program for thermal insulation materials (Insulation LAP) was established in 1979 in response to a request from three private sector thermal insulation trade associations. The purpose of the LAP is to accredit laboratories that produce reliable thermal insulation test data.

Accreditation is available to any organization, such as commercial laboratories, manufacturer's laboratories, university laboratories, and Federal, state, or local government laboratories, that test thermal insulation materials in accordance with the test methods listed in the Appendix.

Products covered: Thermal insulation materials

Period of accreditation: One year

On-site assessment frequency: After initial application and every two years thereafter. Monitoring visits as required.

Proficiency testing:

Each laboratory is sent test samples, data sheets, and an information package containing instructions for specimen preparation, conditioning, mounting, and testing. The completed data sheets are returned to NBS for analysis. The test methods requiring proficiency testing are marked with an asterisk in the list of test methods included in the Application Package sent to each applicant.

The frequency of proficiency testing is twice annually.

Fees: Administrative fee, one-time initial fee, and total test method fee based on the number of test methods selected.

Assessors: Selected from technical experts experienced in the field of thermal insulation testing.

## II. INTRODUCTION

### Background

The U.S. Department of Commerce, National Bureau of Standards (NBS) administers the National Voluntary Laboratory Accreditation Program (NVLAP). NVLAP's function is to accredit public and private testing laboratories based on evaluation of their technical qualifications and competence for conducting specific test methods in specified fields of testing. Accreditation is granted on the basis of conformance with criteria published in the Code of Federal Regulations as part of the NVLAP procedures (15 CFR Part 7). (See Appendix.)

This document is intended for use by staff of accredited laboratories, those seeking accreditation, other laboratory accreditation systems, and others needing information on the requirements for NVLAP accreditation under this LAP. This document is generally included in the NVLAP Application Package along with General Application Forms, Test Method Selection Lists, and other materials needed to apply for or renew accreditation. It presents the administrative and operational procedures and technical requirements of the LAP and should be retained and be readily accessible to laboratory personnel.

### NVLAP Accreditation

Accreditation is granted only after thorough evaluation of the applicant has demonstrated that all NVLAP criteria have been met. The accreditation is formalized through issuance of a Certificate of Accreditation, Scope of Accreditation and publicized by announcement in various government and private media.

NVLAP accreditation is available to commercial laboratories, manufacturer's in-house laboratories, university laboratories, Federal, State, and local government laboratories. Foreign-based laboratories may also be accredited by NBS if they meet the same requirements as domestic laboratories and pay any additional fees required.

### Why NVLAP Accreditation ?

The reasons why a laboratory may wish to be accredited include: legal requirements such as regulations or codes, contract specifications, and the desire to be recognized as being demonstrably competent to meet the needs of its clients.

For accreditation to be meaningful, it must be granted by a clearly credible organization. NVLAP provides an unbiased third party evaluation and recognition of performance as well as expert technical assistance to upgrade laboratory performance.

### Testing Laboratory Defined

NVLAP defines a "testing laboratory" as an organization that provides services to measure, examine, test, calibrate, or otherwise determine the characteristics or performance of products or systems.

### Accreditation Defined

NVLAP accreditation means recognition of a testing laboratory's competence to perform specific test methods in specified fields of testing. It means that the laboratory's quality system, staff, facilities and equipment, calibration procedures, test methods and procedures, records, and test reports, have been evaluated and found to meet NVLAP criteria. NVLAP accreditation does not mean a guarantee (certification) of laboratory performance or product test data; it is a finding of laboratory competence.

For further information about NVLAP, or assistance in understanding and meeting the NVLAP requirements and criteria, please write or call:

NVLAP  
National Bureau of Standards  
ADMIN A531  
Gaithersburg, MD 20899  
Phone: 301-921-3431

### III. ADMINISTRATIVE AND OPERATIONAL REQUIREMENTS

Note: Administrative and operational requirements presented here are generally applicable to all NVLAP programs. Technical and proficiency requirements are specifically applicable to this LAP.

#### LABORATORY CODE NUMBER

Each participating laboratory is assigned a four-digit laboratory code number. The code number is used by the NVLAP staff for identification, filing, recordkeeping, and database management. Participants are requested to put their Lab Code number on all correspondence with NVLAP.

#### ACCREDITATION PERIOD

Accreditation is granted for a period specified in the LAP **Application Package** (usually one year). The accreditation period begins on one of four dates: January 1, April 1, July 1, or October 1. Once a laboratory has been assigned an accreditation date, it retains that date as long as it remains in the program. Accreditation expires and is renewed on that date.

#### RENEWAL

Each participating laboratory will be sent a renewal **Application Package**, well in advance of the expiration date of its accreditation, to allow sufficient time to complete the renewal process. The renewal application contains the same forms used for initial application, and the laboratory need only indicate where changes have occurred from the previous period in personnel, equipment, facilities, or the scope of accreditation desired.

With the exception of an initiation fee for new applicants, the technical requirements and fees are the same as for initial accreditation. The application and fees must be received by NBS prior to expiration of the laboratory's current accreditation to avoid a lapse in accreditation.

#### PUBLICIZING ACCREDITATION STATUS

##### BY NVLAP

NVLAP publishes an annual Directory of Accredited Laboratories. The Directory contains the name and address, scope of accreditation, contact person, and the accreditation renewal date for each accredited laboratory. Supplements to the Directory are published quarterly to cover interim accreditation actions including initial accreditations, renewals, suspensions, terminations, and revocations. The Directory is distributed nationally and internationally to manufacturers, suppliers, retailers, professional and trade associations, code groups, and government agencies.

## BY LABORATORIES

Accredited laboratories are encouraged, within specified limits, to publicize their accredited status. The major restriction is that advertising must not imply product certification by NBS or the U.S. Government. Laboratories and their clients may not reference their accredited status in consumer media, in product advertising, or on product labels, containers or packaging.


A laboratory may cite its accredited status and use NVLAP logos on reports, stationery, and in business and trade publications provided that it is clearly indicated that it is the laboratory which is accredited. NVLAP Lab Bulletin No. 3A provides more detailed guidance on how a laboratory may publicize its accredited status and the statements which may be made. (See Appendix.)

## COMPLIANCE WITH EXISTING LAWS

Accreditation does not relieve the laboratory of the need to observe and comply with existing Federal, State, and local statutes, ordinances, or regulations that may be applicable to its operations, including consumer protection and antitrust laws.

## ACCREDITATION PROCESS

Accreditation is granted following successful completion of a process which includes submission of an application and payment of fees by the laboratory, an on-site assessment, resolution of deficiencies identified during the on-site assessment, participation in proficiency testing, technical evaluation, and administrative review. A diagram of the accreditation process is shown in the figure below.

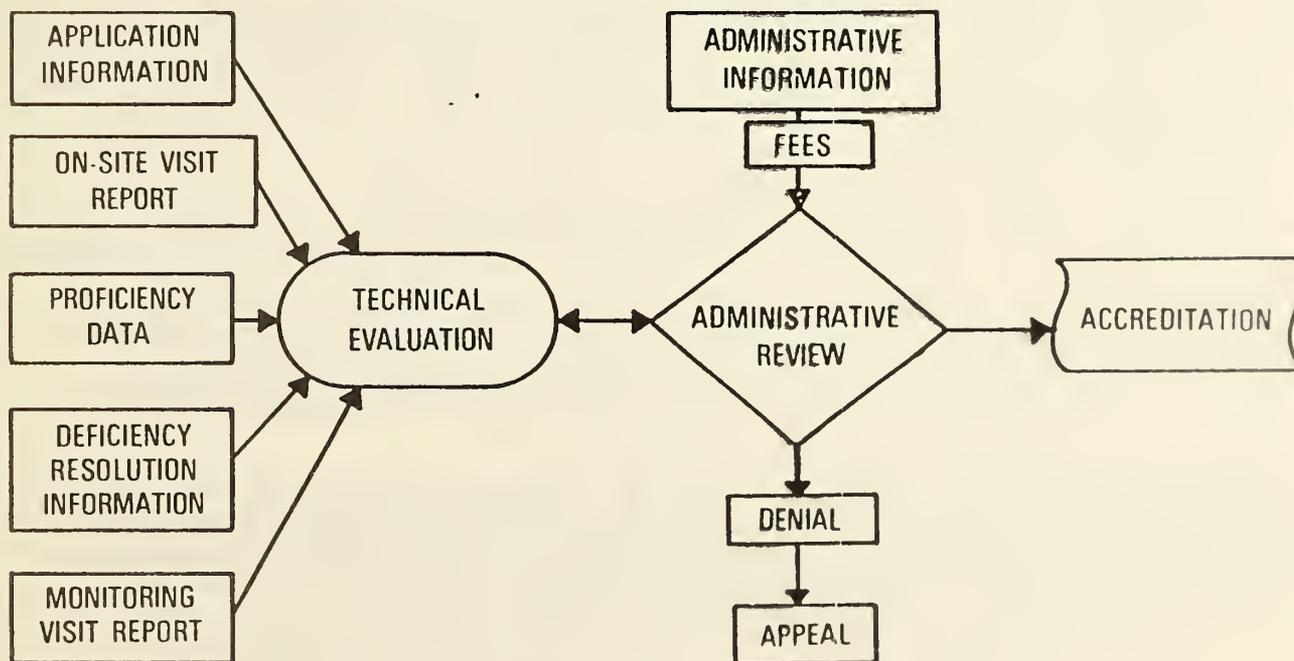

## APPLICATION AND FEES

An Application Package is sent to a laboratory on request. It includes: General Application Forms, a Fee Calculation Sheet, and this document. The General Application Form must be completed and signed by an authorized representative of the laboratory. The authorized representative is one who can act on behalf of the laboratory and commit it to fulfill the NVLAP requirements. Before completing and signing the application, the authorized representative should review all documents and become totally familiar with NVLAP requirements. Although other laboratory staff may be designated to perform activities, such as handling proficiency testing or receiving an assessor, the authorized representative is the only one who can authorize a change in the scope or nature of the application.

In general, the accreditation fee is composed of several parts, some of which are fixed while others depend on the scope of accreditation desired and the specifics of the LAP. The total accreditation fee must be paid before accreditation can be granted. The individual parts of the accreditation fee include, as appropriate: a one-time LAP initiation fee for new applicants, an administrative fee, test method fees, an assessment fee, and proficiency testing fees. The fees for this LAP are shown in the Fee Calculation Sheet included in the LAP Application Package.

The laboratory will be scheduled for an on-site assessment after payment of all required fees and will be notified of any additional information which must be supplied and of any applicable proficiency testing requirements which must be completed for the technical evaluation.

## APPROVED SIGNATORY

Under NVLAP criteria, an accredited laboratory must have one or more individuals or laboratory positions designated as having responsibility for signing "all test reports endorsed with the NVLAP logo." This is the person(s) to whom NVLAP, Laboratory clients, or others would go in case of questions or problems with the report.

There is no formal requirement for nomination or approval of persons or laboratory positions designated as approved signatories. The laboratory should inform NVLAP of its appointments by completing the appropriate sections in the application for accreditation. Approved signatories should be: persons or positions with adequate responsibility or authority within the organization, with adequate and appropriate technical capabilities, and without conflict of interest. The approved signatory may be the authorized representative who is responsible for signing the NVLAP Application Form.

Laboratory test reports carrying the NVLAP logo need not be signed individually by the approved signatory. Test report forms may be preprinted with the required information. Forms that are electronically or computer generated may have the information printed along with the test results.

## TECHNICAL EXPERTS

NVLAP uses Technical Experts (TEs) as assessors and evaluators. These are individuals knowledgeable in the testing field being evaluated. They may be engineers or scientists currently active in the field, consultants, college professors or retired persons. They are selected on the basis of their professional and academic achievements, experience in the field of testing, management experience, and tact in dealing with people. Their services are generally contracted as required; they are not NVLAP staff members.

Assessors are TEs selected to conduct an on-site assessment of a particular laboratory on the basis of how well their individual experience matches the type of testing to be assessed, as well as absence of conflicts of interest. The laboratory has the right to appeal the assignment of an assessor and may request an alternate.

Evaluators are TEs selected to review the record of the laboratory as a whole, including the application, assessment report, deficiencies, corrections to deficiencies, and proficiency test results and, based on this record, to recommend whether or not a laboratory should be accredited. The evaluators are matched to the type of testing being evaluated and are selected to avoid conflicts of interest.

## ON-SITE ASSESSMENT

Before initial accreditation and periodically thereafter, an on-site assessment of each laboratory is conducted to determine compliance with the NVLAP criteria. The assessment is conducted by one or more NVLAP assessors selected on the basis of their expertise in the field of testing to be reviewed. Assessors use checklists developed by NVLAP so that each laboratory receives an assessment comparable to that received by others. However, assessors have considerable latitude to make judgments about a laboratory's compliance with the NVLAP criteria, depending on the assessor's experience and the unique circumstances of the laboratory.

Each laboratory will be contacted to arrange a mutually agreeable date for an assessment. The time needed to conduct an assessment varies, but two days is the norm. Every effort is made to conduct an assessment with as little disruption as possible to the normal operations of the laboratory. During the assessment the assessor will carry out the following functions:

- meet with management and supervisory personnel responsible for the laboratory's activities (for which accreditation is being sought) to review the assessment process with the individuals involved and to set the assessment agenda.
- examine the quality assurance system employed by the laboratory. The assessor may select and trace the history of one or more samples from receipt to final issuance of test reports. The assessor will conduct a thorough review of the laboratory's quality manual or equivalent, evaluate the training program, examine notebooks or records pertaining to the samples, check sample identification and tracking procedures, determine whether the appropriate environmental conditions are maintained, and examine copies of completed test reports.

- review records of periodic internal audits, use of check samples or participation in round robin testing or other similar programs.
- review personnel records including resumes and job descriptions of key personnel, competency evaluations for all staff members who routinely perform the testing for which accreditation is sought, calibration or verification records for apparatus used, test reports, and sample control records.
- observe demonstrations of testing techniques and discuss them with the technical personnel to assure their understanding of the procedures.
- examine major equipment, apparatus, and facilities.

At the conclusion of the assessment, the assessor will conduct an exit briefing to discuss his or her observations with appropriate laboratory staff and call attention to any deficiencies uncovered. A written summary of any deficiencies discussed will be left at the laboratory. The assessor will forward the assessment forms and a written summary to NBS.

If deficiencies have been noted, the laboratory must, within 30 days of the date of this notification provide NVLAP with documentation or certification, by the authorized representative, that the specified deficiencies have been corrected or that specific actions are being taken to correct the deficiencies.

A laboratory applying for initial accreditation may request an extension to complete required corrections.

If any deficiencies are noted at laboratories which are currently accredited, such deficiencies must be corrected within 30 days after notification or the laboratory may face possible revocation, suspension, or expiration of its accreditation. Any test equipment that is identified as out-of-calibration, should not be used until corrective action has been completed. All deficiencies noted for corrective action will be subject to thorough review and verification during subsequent assessments and technical evaluations.

#### MONITORING VISITS

In addition to regularly scheduled assessments, monitoring visits may be conducted by assessors or by NBS staff at any time during the accreditation period. Monitoring visits may occur for cause or on a random selection basis. These visits serve to verify reported changes in the laboratory's personnel, facilities, and operations or to explore possible reasons for poor performance in proficiency testing.

The scope of a monitoring visit may range from checking a few designated items to a complete review. Failure to cooperate with NVLAP assessors will be grounds for initiation of adverse accreditation action. No additional fee is required for the monitoring visit.

## PROFICIENCY TESTING

Proficiency testing is an integral part of the NVLAP accreditation process. Demonstration of appropriate facilities, equipment, personnel, etc. is essential, but may not be sufficient for the evaluation of laboratory competence. The actual determination of test data using special proficiency testing samples provides NVLAP with a way to determine the overall effectiveness of the laboratory.

Proficiency testing is a process for checking actual laboratory testing performance, usually by means of interlaboratory comparisons. Each LAP has unique proficiency testing requirements. The data are analyzed by NVLAP and summary reports of the results are sent back to the participants.

For many test methods, results from proficiency testing are very good indicators of a laboratory's testing capability. Information obtained from proficiency testing helps to identify problems in a laboratory. When problems are found, NVLAP staff members work with the laboratory staff to solve them. If problems with the test method are suspected, NVLAP provides information to the appropriate standards-writing bodies.

The specific proficiency testing requirements for this LAP are included in Section V of this document.

## TECHNICAL EVALUATION

After a laboratory has completed all the technical requirements of a LAP and is ready for an accreditation action, a final technical evaluation is conducted by experts chosen for their experience and knowledge of the pertinent test methods. They review records on each applicant laboratory and base their evaluation on:

- information provided on the application;
- on-site assessment reports;
- actions taken by the laboratory to correct deficiencies;
- results of proficiency testing; and
- information from any monitoring visits of the laboratory.

If the technical evaluation reveals additional deficiencies, written notification describing them will be made to the laboratory. The laboratory must respond within 30 days of such notification and provide documentation or certification by the authorized representative that the specified deficiencies have been corrected. Clarification of some issues may be requested by telephone. All deficiencies must be corrected before accreditation can be granted or renewed.

## ADMINISTRATIVE REVIEW

After the technical evaluation has been completed, the NVLAP staff prepares an administrative recommendation that the laboratory either be granted or denied accreditation. This recommendation is based on a review of the technical evaluation and other records to ensure that all NVLAP technical, financial and administrative obligations have been satisfied.

## ACCREDITATION ACTIONS

Acting for the Director of NBS, the Director of the NBS Office of Product Standards Policy makes the following decisions.

Accreditation If accreditation is recommended, the recommendation forms the basis for granting accreditation. A **Certificate of Accreditation** will be issued to the laboratory.

Denial If denial is recommended, the laboratory is notified of a proposal to deny accreditation and the reason(s) therefor.

Suspension If a laboratory is found to have violated the terms of its accreditation, the accreditation can be suspended. The laboratory will be notified of the reasons for and conditions of the suspension and the action(s) that the laboratory must take to have accreditation reinstated.

Revocation If a laboratory is found to have violated the terms of its accreditation, the laboratory is notified of a proposal to revoke accreditation and the reasons therefor. The laboratory may be given the option of voluntarily terminating accreditation. If accreditation is revoked, the laboratory must return its **Certificate of Accreditation** and cease use of the NVLAP logo on any of its reports, other correspondence, or advertising.

If denial or revocation has been proposed, the laboratory may request a hearing, under United States Code 5 U.S.C. 556, within 30 days of the date of receipt of the notification. If a hearing is not requested, the action becomes final upon the expiration of that 30-day period.

After a participant's accreditation has been terminated, whether voluntarily or through adverse action, the accreditation certificate must be returned to NVLAP. If a laboratory elects not to renew or wishes to voluntarily terminate its accreditation at any time, the notification of such intention should be forwarded to NBS in writing.

#### IV. TECHNICAL REQUIREMENTS

The requirements discussed in this section interpret the NVLAP criteria for application to the Insulation LAP. These requirements do not supersede the published NVLAP criteria which are included in the Appendix.

##### SCOPE OF THE LAP

The Insulation LAP covers tests for thermal insulation materials. The test methods for which a laboratory may seek accreditation are listed in the Appendix. Other test methods may be added to the LAP, upon request, if they are found to be appropriate.

##### QUALITY ASSURANCE SYSTEM

The key to a properly functioning organization is that it has and maintains a system of procedures and practices which assure the quality of its services. To qualify for accreditation, an applicant must demonstrate that its quality systems ensure the technical integrity of its work.

##### DOCUMENTATION

A laboratory must have up-to-date documentation which thoroughly describes all its procedures and practices. The written descriptions should contain such items as the method of implementation, responsible personnel, recordkeeping system, operating procedures, procedures to employ in the event of unusual or non-standard circumstances, and scheduling. Written descriptions should include at least the following topics:

- Organizational chart;
- Laboratory facilities and scope of services offered;
- Job/position description for all personnel;
- Personnel training procedures;
- Personnel competency assurance procedures;
- Test equipment inventory;
- Test equipment calibration, verification, and maintenance practices;
- Test performance plan;
- Specimen selection, handling, analysis, control, and identification;
- Data handling and reporting;
- Internal checks and audits;
- External standardization practices;
- Reference standards and/or materials; and
- Subcontracting practices and procedures for assuring quality

This documentation should be in the form of a manual but may consist of individual sheets in various locations throughout the facility. If individual sheets are used, a central reference document must be available to indicate where the sheets may be found. The documentation must be in a format and style which can be easily understood by technicians. It must be readily accessible to all staff members.

## PERSONNEL

### Training:

Each new staff member must be trained for assigned duties and existing staff members must be retrained when testing equipment and/or protocols are changed or they are assigned new responsibilities. Each staff member must receive (or have had) training for assigned duties either through on-the-job training, formal classroom sessions or through technician certification programs.

For the Insulation LAP, the training program must include the applicable portions of the following, as a minimum:

#### Thermal Resistance Measurements:

- General Requirements of the test method;
- Specimen preparation techniques including dealing with very compressible materials;
- Techniques for installation of thermocouples in thermal measurement apparatus;
- Theory of heat transfer measurements, including edge guarding, and effects of thickness, density, and orientation.

#### Corrosion Tests:

- General Requirements of the test method;
- Degreasing, cleaning, and corrosion evaluation techniques for metal coupons.

#### Flammability Tests:

- General Requirements of the test method;
- Specimen preparation techniques;
- Understanding of and ability to interpret the results of surface flammability and smoldering combustion tests.

#### Dimensional Stability Tests:

- General Requirements of the test method;
- Specimen preparation techniques including dealing with compressible materials;
- Procedure and technique for blowing and shaking loose-fill cellulosic materials in conducting settled density test and making associated calculations.

### Vapor Barrier Tests:

General Requirements of the test method;  
Procedures for using template and attaching specimen to dish,  
weighing samples, and calculating water vapor transmission.

### Strength Tests:

General Requirements of the test method;  
Operation of the tensile/compression testing machine.

### Competency:

In addition to training, the supervisor must evaluate the competency of each staff member by observing the performance of each testing protocol each staff member is authorized to conduct. The performance observation must be conducted annually by the immediate supervisor or his designee. A record of the staff member's performance must be placed in the personnel file, dated and signed by the supervisor.

### Technical Director:

The laboratory technical director shall be a professional experienced in the testing area for which accreditation is desired. This individual should have the technical competence and the supervisory responsibility to direct the work of professionals and technicians in the appropriate area. Responsibility for the quality assurance program may reside with the technical director or with another individual having knowledge and experience in quality assurance who has a direct line of communication to the technical director and other organizational management.

The assessor will review resumes or other information to substantiate the qualifications of the Technical Director and all key individuals.

Any organizational or personnel changes that could affect the performance of the testing service (e.g., Technical Director, technical supervision, responsibility for quality assurance program) shall be reported to NVLAP within 30 calendar days of such change.

### EQUIPMENT AND FACILITIES

A laboratory must have adequate equipment to perform the type(s) of testing for which capability is claimed. This includes adequate space to perform the testing, environmental controls, adequate testing equipment, adequate safety systems and either properly calibrated laboratory standards or access to the services of a competent calibration laboratory.

## EQUIPMENT MAINTENANCE AND CALIBRATION

All equipment used in the testing of the thermal insulation materials and to perform quality control must be adequately maintained so that it can accomplish the required measurements.

Measurement or quality control equipment that is inherently subject to change due to use or passage of time, must be periodically calibrated. Calibration means comparison with a reference standard so that the performance of a measuring instrument may be determined with sufficient accuracy.

Calibrations of equipment may be performed by the laboratory or by an external calibration service. All calibrations and characterizations must be done against reference standards that are traceable to national standards maintained by NBS or by an equivalent foreign national standards authority. To be traceable means the ability to show that appropriate documented actions were taken to compare (either directly or indirectly) a reference standard with a national standard.

The reference standards used and the environmental conditions at the time of calibration must be documented for all calibrations. Calibration records and evidence of the traceability of the reference standards used must be made available for inspection during the on-site visit.

Testing equipment or verification records should include the following: equipment name or description; model, style, or serial number; manufacturer; notation of all equipment variables requiring verification; the range of verification; the resolution of the instrument and its allowable error; verification date and schedule; date and result of last calibration; identity of the laboratory individual or external service responsible for calibration; source of reference standard and traceability.

The equipment used for conducting the tests in the Insulation LAP must be maintained and calibrated (or verified) in accordance with the manufacturer's recommendation, as specified in the test method, or as specified below, whichever frequency is greater.

<u>Apparatus/Instrumentation</u>	<u>Calibration or Verification Frequency</u>
balances	annually
tensile/compression testing machines (load cells)	annually
drying ovens	annually
furnaces	annually
dimensional measurement devices (calipers, micrometers, etc.)	annually
heat flux meters	annually
pyrometers	annually

automatic data logging and readout instrumentation	semi-annually
ammeters, ohmmeters, voltmeters, wattmeters	semi-annually
potentiometers	semi-annually
thermocouples and related instrumentation	semi-annually
environmental control apparatus	quarterly
humidity cabinets	quarterly
cold boxes	quarterly
radiant panel	as per test method
heat flow meters	as per test method
guarded hot plates	as per test method

## RECORDKEEPING

A laboratory must maintain a functional recordkeeping system. This means that records must be easily accessible, in some logical order and contain complete information on the subject. Records covering the following items are required and will be reviewed during the on-site visit either in total or by selected sampling:

- Staff training dates and results;
- Staff competency review dates and results;
- Testing equipment calibration and maintenance;
- Results of incoming inspection of materials;
- Comprehensive logs of test activities;
- Results of internal and external equipment checks, measurement assurance programs, quality audits, etc.;
- Test data and reports; and
- Tracking and logging of samples tested.

Sample tracking and logging records should trace the movement of each sample through the testing facility from its receipt through all the tests performed to the final test report. Dates, times, condition of item and personnel involved should all be included.

## FINAL REPORT

The final report to the client must include:

- Name and address of laboratory;
- Pertinent dates and identifying numbers;
- Client name;
- Description or identification of each sample;
- Identification of the test method, procedures, or specifications;
- Identification of known deviations, additions to, or exclusions from the test method;
- Measurements, examinations, or derived results, and identification of test anomalies;

- A statement, if necessary, as to whether or not the test results comply with the requirements of product or project specifications;
- Signature of person having technical responsibility for the test report; and
- All other items required by the test method.

Records of these reports must be maintained for at least three years.

## V. PROFICIENCY TESTING

Proficiency testing is an integral requirement of the NVLAP evaluation process. NBS either conducts the proficiency testing program for the LAP or determines if a collaborative reference program or round-robin testing program exists which can meet the testing requirements for the LAP. The test methods for which proficiency testing is required for the Insulation LAP are indicated by an asterisk in the list of test methods in the Appendix.

Twice annually each laboratory is sent test samples, data sheets, and an information package containing instructions for specimen preparation, conditioning, mounting, and testing. Although it is generally required that the test be conducted in accordance with the applicable test method, the number of replicate measurements, special conditions of temperature and humidity, and other parameters are sometimes specified to ensure uniformity in procedures and test conditions among participants. Completed data sheets must be returned to NBS for analysis by the date specified on the sheets.

## APPENDICES

NVLAP Accreditation Criteria

NVLAP Lab Bulletin No. 3A

Test Method List



## NVLAP Accreditation Criteria

### SUBPART D - CONDITIONS AND CRITERIA FOR ACCREDITATION

#### Sec. 7.31 Application of accreditation conditions and criteria.

(a) To become accredited and maintain accreditation, a laboratory must meet the conditions for accreditation set out in Section 7.32 and the criteria set out in Section 7.33 as tailored for specific LAPs.

(b) The conditions leading to accreditation include acceptance of the responsibilities of an accredited laboratory and requirements for information disclosure.

(c) The criteria are tailored and interpreted for the test methods, types of test methods, products, services or standards of the relevant LAP. These tailored criteria are the technical requirements for accreditation developed through the procedures of Section 7.15.

(d) In applying the conditions, criteria, and technical requirements for accreditation, the Director of OPSP shall not:

- (1) Prohibit accreditation solely on the basis of a laboratory's affiliation or nonaffiliation with manufacturing, distributing, or vending organizations, or because the laboratory is a foreign firm; or
- (2) Develop, modify, or promulgate test methods, standards, or comparable administrative rules.

#### Sec. 7.32 Conditions for accreditation.

(a) To become accredited and maintain accreditation, a laboratory shall agree in writing to:

- (1) Be assessed and evaluated initially and on a periodic basis;
- (2) Demonstrate, on request, that it is able to perform the tests representative of those for which it is seeking accreditation;
- (3) Pay all relevant fees;
- (4) Participate in proficiency testing as required.
- (5) Be capable of performing the tests for which it is accredited according to the latest version of the test method within one year after its publication or within another time limit specified by the Director of OPSP;
- (6) Limit the representation of the scope of its accreditation to only those tests or services for which accreditation is granted;
- (7) Limit all its test work or services for clients to those areas where competence and capacity are available;
- (8) Limit advertising of its accredited status to letterheads, brochures, test reports, and professional, technical, trade, or other laboratory services publications, and use the NVLAP logo under guidance provided by the Director of OPSP;
- (9) Inform its clients that the laboratory's accreditation or any of its test reports in no way constitutes or implies product certification, approval, or endorsement by NBS;
- (10) Maintain records of all actions taken in response to testing complaints for a minimum of one year;

- (11) Maintain an independent decisional relationship between itself and its clients, affiliates, or other organizations so that the laboratory's capacity to render test reports objectively and without bias is not adversely affected;
- (12) Report to the Director of OPSP within 30 days any major changes involving the location, ownership, management structure, authorized representative, approved signatories, or facilities of the laboratory; and
- (13) Return to the Director of OPSP the certificate of accreditation for possible revision or other action should it:
  - (i) be requested to do so by the Director of OPSP;
  - (ii) voluntarily terminate its accredited status; or
  - (iii) become unable to conform to any of these conditions or the applicable criteria of Section 7.33 and related technical requirements.

(b) To become accredited and maintain accreditation, a laboratory shall supply, upon request, the following information:

- (1) Legal name and full address;
- (2) Ownership of the laboratory;
- (3) Organization chart defining relationships that are relevant to performing testing covered in the accreditation request;
- (4) General description of the laboratory, including its facilities and scope of operation;
- (5) Name and telephone number of the authorized representative of the laboratory;
- (6) Names or titles and qualifications of laboratory staff nominated to serve as approved signatories of test reports that reference NVLAP accreditation; and
- (7) Other information as may be needed for the specific LAP(s) in which accreditation is sought.

#### Sec. 7.33 Criteria for accreditation.

- (a) Quality System. (1) The laboratory shall operate under an internal quality assurance program appropriate to the type, range, and volume of work performed. The quality assurance program must be designed to ensure the required degree of accuracy and precision of the laboratory's work and should include key elements of document control, sample control, data validation, and corrective action. The quality assurance program must be documented in a quality manual or equivalent (e.g., operations notebook) which is available for use by laboratory staff. A person(s) must be identified as having responsibility for maintaining the quality manual.
- (2) The quality manual must include as appropriate:
  - (i) The laboratory's quality assurance policies including procedures for corrective action for detected test discrepancies;
  - (ii) Quality assurance responsibilities for each function of the laboratory;
  - (iii) Specific quality assurance practices and procedures for each test, type of test, or other specifically delineated function performed;
  - (iv) Specific procedures for retesting, control charts, reference materials, and interlaboratory tests; and
  - (v) Procedures for dealing with testing complaints.
- (3) The laboratory shall periodically review its quality assurance system by or on behalf of management to ensure it's continued effectiveness. These reviews must be recorded with details of any corrective action taken.

- (b) Staff. (1) The laboratory shall:
- (i) Be staffed by individuals having the necessary education, training, technical knowledge, and experience for their assigned functions; and
  - (ii) Have a job description for each professional, scientific, supervisory and technical position, including the necessary education, training, technical knowledge, and experience.
- (2) The laboratory shall document the test methods each staff member has been assigned to perform.
- (3) The laboratory shall have a description of its training program for ensuring that new or untrained staff are able to perform tests properly and uniformly to the requisite degree of precision and accuracy.
- (4) The laboratory shall be organized:
- (i) So that staff members are not subjected to undue pressure or inducement that might influence their judgment or results of their work; and
  - (ii) In such a way that staff members are aware of both the extent and the limitation of their area of responsibility.
- (5) The laboratory shall have a technical manager (or similar title) who has overall responsibility for the technical operations of the laboratory.
- (6) The laboratory shall have one or more signatories approved by the Director of OPSP to sign test reports that reference NVLAP accreditation. Approved signatories shall:
- (i) Be competent to make a critical evaluation of test results; and
  - (ii) Occupy positions within the laboratory's organization which makes them responsible for the adequacy of test results.
- (c) Facilities and Equipment. (1) The laboratory shall be furnished with all items of equipment and facilities for the correct performance of the tests and measurements for which accreditation is granted and shall have adequate space, lighting, and environmental control, and monitoring to ensure compliance with prescribed testing conditions.
- (2) All equipment must be properly maintained to ensure protection from corrosion and other causes of deterioration. Instructions for a proper maintenance procedure for those items of equipment which require periodic maintenance must be available. Any item of equipment or component thereof which has been subjected to overloading or mishandling, gives suspect results, or has been shown by calibration or otherwise to be defective, must be taken out of service and clearly labelled until it has been repaired. When placed back in service, this equipment must be shown by test or calibration to be performing its function satisfactorily.
- (3) Records of each major item of equipment must be maintained. Each record must include:
- (i) The name of the item of equipment;
  - (ii) The manufacturer's name and type, identification and serial number;
  - (iii) Date received and date placed in service;
  - (iv) Current location, where appropriate;
  - (v) Details of maintenance; and
  - (vi) Date of last calibration, next calibration due date, and calibration report references.

(d) Calibration. The laboratory shall:

- (1) Calibrate new testing equipment before putting it into service;
- (2) Recalibrate, at regular intervals, in-service testing equipment with the calibration status readily available to the operator;
- (3) Perform checks of in-service testing equipment between the regular calibration intervals, where relevant;
- (4) Maintain adequate records of all calibrations and recalibrations; and
- (5) Provide traceability of all calibrations and reference standards of measurement where these standards exist. Where traceability of measurements to primary (national or international) standards is not applicable, the laboratory shall provide satisfactory evidence of the accuracy or reliability of test results (e.g., by participation in a suitable program of interlaboratory comparison).

(e) Test Methods and Procedures. The laboratory shall:

- (1) Conform in all respects with the test methods and procedures required by the specifications against which the test item is to be tested, except that whenever a departure becomes necessary for technical reasons the departure must be acceptable to the client and recorded in the test report;
- (2) Have data to prove that any departures from standard methods and/or procedures due to apparatus design or for other reasons do not detract from the expected or required precision of the measurement;
- (3) Maintain a test plan for implementing testing standards and procedures including adequate instructions on the use and operation of all relevant equipment, on the handling and preparation of test items (where applicable), and on standard testing techniques where the absence of such instructions could compromise the test. All instructions, testing standards, specifications, manuals, and reference data relevant to the work of the laboratory must be kept up-to-date and made readily available to the staff;
- (4) Maintain measures for the detection and resolution of in-process testing discrepancies for manual and automatic test equipment and electronic data processing equipment, where applicable;
- (5) Maintain a system for identifying samples or items to be tested, which remains in force from the date of receipt of the item to the date of its disposal, either through documents or through marking to ensure that there is no confusion regarding the identity of the samples or test items and the results of the measurements made; and
- (6) Maintain rules for the receipt, retention, and disposal of test items, including procedures for storage and handling precautions to prevent damage to test items which could invalidate the test results. Any relevant instructions provided with the tested item must be observed.

(f) Records. The laboratory shall:

- (1) Maintain a record system which contains sufficient information to permit verification of any issued report;
- (2) Retain all original observations, calculations and derived data, and calibration records for one year unless a longer period is specified; and
- (3) Hold records secure and in confidence, as required.

- (g) Test Reports. (1) The laboratory shall issue test reports of its work which accurately, clearly, and unambiguously present the specified test results and all required information. Each test report must include the following information as applicable:
- (i) Name and address of the laboratory;
  - (ii) Identification of the test report by serial number, date, or other appropriate means;
  - (iii) Name and address of client;
  - (iv) Description and identification of the test specimen, sample, or lot of material represented;
  - (v) Identification of the test specification, method, or procedure used;
  - (vi) Description of sampling procedure, if appropriate;
  - (vii) Any deviations, additions to, or exclusions from the test specifications;
  - (viii) Measurements, examinations, and derived results supported by tables, graphs, sketches, and photographs, as appropriate, and any failures identified;
  - (ix) A statement of measurement uncertainty where relevant;
  - (x) Identification of the organization and the person accepting technical responsibility for the test report and date of issue;
  - (xi) A statement that the report must not be reproduced except in full with the approval of the laboratory; and
  - (xii) A statement to the effect that the test report relates only to the items tested.
- (2) The laboratory shall issue corrections or additions to a test report only by a further document suitably marked, e.g. "Supplement to test report serial number .....", which meets the relevant requirements of Section 7.33(g)(1).
- (3) The laboratory shall retain a copy of each test report issued for one year unless a longer period is specified by the Director of OPSP.
- (4) The laboratory shall ensure that all test reports endorsed with the NVLAP logo are signed by an approved signatory.





# Bulletin

Lab Bulletin No. 3A

January 1, 1985

## INFORMING THE PUBLIC OF YOUR ACCREDITATION STATUS

### Summary

This Bulletin supersedes NVLAP Lab Bulletin No. 3 dated October 1, 1981. It reflects significant changes made to the NVLAP procedures (Title 15, Part 7, of the Code of Federal Regulations) which became effective on December 10, 1984.

The Bulletin is addressed primarily to personnel at accredited laboratories who are responsible for communicating the laboratory's accreditation status to clients and the public, through advertising, issuance of test reports, use of the NVLAP logo, etc.

The Bulletin's purpose is to "provide guidance on referencing the laboratory's accredited status, and use of the NVLAP logo by the laboratory and its clients," in accordance with provisions of the NVLAP Procedures.

### Background

NVLAP was established to assist industry and government in identifying competent testing laboratories. NVLAP accreditation means that a laboratory is competent to perform specific test methods in selected fields of testing. The NVLAP Procedures are the bases upon which the entire program operates and accomplishes accreditation of laboratories. Parts A and B of the Procedures provide general information and the method by which a new Laboratory Accreditation Program (LAP), in a new field of testing, may be requested and established. Parts C and D of the Procedures, of more concern to accredited laboratories, describe how a laboratory becomes accredited and the conditions and criteria for initial and continued accreditation. This Bulletin is concerned principally with issues in Part D of the Procedures.

Requirements and Guidance

To become accredited and maintain accreditation a laboratory shall:

limit the representation of the scope of its accreditation to only those tests or services for which accreditation is granted

A laboratory accredited by NVLAP may use the following statement on its letterheads and in trade or other publications: "Accredited by the National Bureau of Standards, National Voluntary Laboratory Accreditation Program for selected test methods for --(identify product or service area(s))." This statement could, for example, be placed at the bottom of the laboratory letterhead.

A laboratory's letterhead containing a reference to its NVLAP accreditation may be used in any direct solicitation for business from potential customers. It is recommended that a copy of the NVLAP Certificate and Scope of Accreditation be appended to such a solicitation.

To become accredited and maintain accreditation a laboratory shall:

limit advertising of its accredited status to letterheads, brochures, test reports, and professional, technical, trade, or other laboratory services publications, and use the NVLAP logo under guidance provided by NBS

A statement about NVLAP accreditation and the NVLAP logo may be used on reports and data sheets containing test data obtained by a laboratory provided the tests or services are performed in accordance with the terms of its accreditation. The NVLAP logo may not be used on test reports or data sheets during any period of suspended or expired accreditation or after voluntary or involuntary termination of accreditation.

The nature or type of product advertising prohibited by NVLAP procedures includes any advertising that is intended to encourage a consumer to purchase a product because it was tested by an accredited laboratory, whether that advertising appears in consumer media, the business media, or at a point of sale to consumers.

News stories and advertising by laboratories of their accredited status in the trade press is not only permissible but encouraged. The use of advertisements in the trade press is consistent with NVLAP procedures.

The "consumer media" to be avoided include popular periodicals such as Time, Good Housekeeping, etc., and newspapers such as the Washington Post or the New York Times. The term "consumer media" does not include business publications such as Barron's, or the Wall Street Journal which are oriented to the business community and in which products per se normally are not advertised.

To become accredited and maintain accreditation a laboratory shall:

inform its clients that the laboratory's accreditation or any of its test reports in no way constitutes or implies product certification, approval, or endorsement by NBS

Laboratory accreditation by NBS confers recognition that a laboratory has been found competent to perform specific test methods or services in a selected field(s) of testing. Laboratories must avoid all inference that accreditation under NVLAP carries with it an endorsement, approval, or recommendation of the products tested by the laboratories.

To become accredited and maintain accreditation a laboratory shall:

assure that all test reports endorsed with the NVLAP logo are signed by an approved signatory

An approved signatory is an officer or employee of the laboratory, identified by name or position, who has been accepted by NVLAP as being responsible for the issuance of test reports under this condition of NVLAP accreditation. A laboratory seeking initial accreditation or reaccreditation must specify (a) one or more individuals, or (b) position(s) within the organization for which it requests acceptance as an approved signatory.

Computer or machine generated test reports that contain the NVLAP logo need not be signed but must have the printed name of the approved signatory.

#### Questions About Accreditation

If you have questions about what is an acceptable method of advertising in areas not specifically covered in this Lab Bulletin or about the propriety or acceptability of a particular statement, advertising media, or use of information about your NVLAP accreditation status, please contact NVLAP before your publicity program is implemented.

Call 301-921-3431 or

Send your questions to:

Harvey W. Berger  
Associate Manager, Laboratory Accreditation  
National Bureau of Standards  
ADMIN A531  
Gaithersburg, MD 20899



## APPENDIX

## TEST METHOD LIST

<u>NVLAP Test Method Code</u>	<u>Test Method Designation</u>	<u>Test Method Short Title</u>
01/C01	ASTM C739 (para. 10.7 in 80 version)	Corrosiveness; Cellulosic fiber (loose-fill)
01/C02	HH-I-515 (para. 4.8.5 in D version, Amendment 1)	Corrosiveness; Cellulosic fiber (loose-fill)
01/C03	California Energy Commission tests for insulating materials: Corrosiveness - Mineral fiber blankets and loose-fill	
01/D01	ASTM C136	Sieve or screen analysis
01/D02	ASTM C167	Thickness and density; Blanket and batt
01/D03	ASTM C209 (para. 6 in 72 version)	Thickness; Board (cellulosic fiber)
01/D04	ASTM C209	Water absorption, 2 hour;
01/D05	ASTM C209 (para. 13 in 72 version) by D1037 (para. 100-106 in 78 version)	Water absorption, 24 hour; Board (cellulosic fiber)
01/D06	ASTM C209 (para. 14 in 72 version) by D1037 (para. 107-110 in 72 version)	Linear expansion; Board (cellulosic fiber)
01/D07	ASTM C272	Water absorption; Core materials
01/D08	ASTM C302	Density; Preformed pipe insulation
01/D09	ASTM C303	Density; Preformed block insulation
01/D11	ASTM C356	Linear shrinkage; Soaking heat; Preformed high temperature insulation
01/D12	ASTM C411	Hot-surface performance; High temperature insulation
01/D13	ASTM C519	Density; Loose-fill (fibrous)
01/D14	ASTM C520	Density; Granular loose-fill
01/D15	ASTM D756	Weight and shape changes; Accelerated service (proc. A); Plastics

01/D16	ASTM D756	Weight and shape changes; Accelerated service (proc. B); Plastics
01/D17	ASTM D756	Weight and shape changes; Accelerated service (proc. E); Plastics
01/D18	ASTM D1622	Apparent density; Rigid cellular plastics
01/D19	ASTM D2126	Response to thermal and humid aging (proc. B); Rigid cellular plastics
01/D20	ASTM D2126	Response to thermal and humid aging (proc. D); Rigid cellular plastics
01/D21	ASTM D2126	Response to thermal and humid aging (proc. E); Rigid cellular plastics
01/D22	ASTM D2126	Response to thermal and humid aging (proc. F); Rigid cellular plastics
01/D23	ASTM D2842	Water absorption; Rigid cellular plastics
01/D24	ASTM C739 (para. 10.5 in 80 version)	Moisture absorption; Cellulosic fiber (loose-fill)
01/D25	HH-I-515 (para. 4.8.3 in D version, Amendment 1)	Moisture absorption; Cellulosic fiber (loose-fill)
* 01/D26	HH-I-515 (para. 4.8.1 in D version, Amendment 1)	Settled density; Cellulosic fiber (loose-fill)
01/D27	ASTM D2126	Response to thermal and humid aging (proc. C); Rigid cellular plastics
01/D28	ASTM D2126	Response to thermal and humid aging (proc. G); Rigid cellular plastics
01/D29	California Energy Commission tests for insulating materials: Installed compressed thickness	
01/F01	TAPPI T461	Flame Resistance; Paper and paperboard
* 01/F02	ASTM E84	Surface burning characteristics; Building materials
01/F05	ASTM E136	Behavior of Materials in a Vertical Tube Furnace
01/F06	ASTM C739 (para. 10.4 in 80 version)	Flame resistance permanency; Cellulosic fiber (loose-fill)

* 01/F07	HH-I-515 (para. 4.8.7 in D version, Amendment 1)	Critical radiant flux; Radiant Panel (cellulosic fiber, loose-fill)
* 01/F08	HH-I-515 (para. 4.8.8 in D version, Amendment 1)	Smoldering combustion; Cellulosic fiber (loose-fill)
01/S01	ASTM C165	Compressive properties; Thermal insulation (proc. A)
01/S02	ASTM C203	Breaking load/flexural strength; Preformed block insulation
01/S03	ASTM C209 (para. 9 in 72 version)	Transverse strength; Board (cellulosic fiber)
01/S04	ASTM C209 (para. 10 in 72 version)	Deflection at specified load; Board (cellulosic fiber)
01/S05	ASTM C209 (para. 11 in 72 version)	Tensile strength; Parallel to surface; Board (cellulosic fiber)
01/S06	ASTM C209 (para. 12 in 72 version)	Tensile strength; Perpendicular to surface
01/S07	ASTM C273	Shear test; Sandwich construction
01/S08	ASTM C446	Breaking load/modulus of rupture; Preformed pipe insulation
01/S09	ASTM D781	Puncture test; Paperboard and fiberboard
01/S10	ASTM D828	Tensile breaking strength; Paper and paperboard
01/S11	ASTM D1621	Compressive properties; Rigid cellular plastics (proc. A-Crosshead)
01/S12	California Energy Commission tests for insulating materials: Bond strength - Spray applied cellulose	
01/S13	California Energy Commission tests for insulating materials: Bond deflection - Spray applied cellulose	
01/S14	California Energy Commission tests for insulating materials: Air erosion - Spray applied cellulose	
* 01/T01	ASTM C177	Thermal transmission properties; Low-temperature guarded hot plate
* 01/T04	ASTM C236	Thermal conductance; Guarded hot box

01/T05	ASTM C335	Thermal conductivity; Pipe insulation
* 01/T06	ASTM C518	Thermal transmission properties; Heat flow meter
01/T09	ASTM C653	Thermal resistance (Rec. Practice); Blanket (mineral fiber)
01/T10	ASTM C687	Thermal resistance (Rec. Practice); Loose-fill (fibrous)
01/V02	TAPPI T419	Starch in paper; Qualitative test
01/V03	ASTM D2020	Mildew (fungus) resistance; Paper and paperboard
01/V04	ASTM E96	Water vapor transmission; Thin sheets (proc. A)
01/V05	HH-I-515 (para. 4.8.6 in D version, Amendment 1)	Fungus; Cellulosic fiber (loose-fill)
01/V06	HH-I-515 (para. 4.8.9 in D version, Amendment 1)	Starch; Cellulosic fiber (loose-fill)

U.S. DEPT. OF COMM. <b>BIBLIOGRAPHIC DATA SHEET</b> <i>(See instructions)</i>	<b>1. PUBLICATION OR REPORT NO.</b> NBSIR-85/3184	<b>2. Performing Organ. Report No.</b>	<b>3. Publication Date</b> June 1985
<b>4. TITLE AND SUBTITLE</b> Insulation LAP Handbook: Operational and Technical Requirements for the Laboratory Accreditation Program for Thermal Insulation Materials			
<b>5. AUTHOR(S)</b> Wiley A. Hall, Jr., Robert L. Gladhill, Jeffrey Horlick, Harvey W. Berger			
<b>6. PERFORMING ORGANIZATION</b> <i>(If joint or other than NBS, see instructions)</i>  NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE <del>WASHINGTON, D.C. 20334</del> Gaithersburg, MD 20899		<b>7. Contract/Grant No.</b>	<b>8. Type of Report &amp; Period Covered</b>
<b>9. SPONSORING ORGANIZATION NAME AND COMPLETE ADDRESS</b> <i>(Street, City, State, ZIP)</i>			
<b>10. SUPPLEMENTARY NOTES</b>  <input type="checkbox"/> Document describes a computer program; SF-185, FIPS Software Summary, is attached.			
<b>11. ABSTRACT</b> <i>(A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here)</i>  This document explains the operation and technical requirements of the Laboratory Accreditation Program (LAP) for Thermal Insulation Materials (Insulation LAP). All of the steps leading to accreditation are discussed. Technical requirements are explained indicating how the NVLAP criteria are applied.  It is intended for use by staff of accredited laboratories, those seeking accreditation, other laboratory accreditation systems, and others needing information on the requirements for NVLAP accreditation under this LAP.			
<b>12. KEY WORDS</b> <i>(Six to twelve entries; alphabetical order; capitalize only proper names; and separate key words by semicolons)</i> accreditation; assessment; laboratory; thermal insulation materials; proficiency testing			
<b>13. AVAILABILITY</b>  <input checked="" type="checkbox"/> Unlimited <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS <input type="checkbox"/> Order From Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402.  <input checked="" type="checkbox"/> Order From National Technical Information Service (NTIS), Springfield, VA. 22161		<b>14. NO. OF PRINTED PAGES</b>  31	<b>15. Price</b>  \$8.50





